

Qualitative Analysis of Teeth and Evaluation of Amalgam Elements Penetration into Dental Matrix Using Laser Induced Breakdown Spectroscopy

Meisam Gazmeh¹, Maryam Bahreini^{1*}, Seyed Hassan Tavassoli¹, Mohammad Asnaashari²

¹Laser and Plasma Research Institute, Shahid Beheshti University, G. C., Evin, Tehran, 1983963113, Iran

²Laser Application in Medical Sciences Research Center, Shahid Beheshti University of Medical Sciences, Tehran, Iran

Abstract:

Introduction: In this study, laser induced breakdown spectroscopy (LIBS) is used for qualitative analysis of healthy and carious teeth. The technique of laser ablation is receiving increasing attention for applications in dentistry, specifically for the treatment of teeth such as drilling of micro-holes and plaque removal.

Methods: A quality-switched (Q-switched) Neodymium-Doped Yttrium Aluminium Garnet (Nd:YAG) laser operating at wavelength of 1064 nm, pulse energy of 90 mJ/pulse, repetition rate of 2Hz and pulse duration of 6 ns was used in this analysis. In the process of ablation a luminous micro-plasma is normally generated which may be exploited for on-line elemental analysis via laser induced breakdown spectroscopy technique. We propose laser induced breakdown spectroscopy as a rapid, in situ and easy method for monitoring drilling process.

Results: The results of elemental analysis show the presence of some trace elements in teeth including P, Ca, Mg, Zn, K, Sr, C, Na, H, O and the permeability of some amalgam (teeth filling materials) elements including Hg, Ag, Cu and Sn into dental matrix.

Conclusion: This study addresses the ability of LIBS in elemental analysis of teeth and its feasibility in acute identification of healthy and carious teeth during drilling process for future clinical applications.

Keywords: spectroscopy; tooth; carious; amalgam.

Please cite this article as follows:

Gazmeh M, Bahreini M, Tavassoli SA, Asnaashari M. Qualitative Analysis of Teeth and Evaluation of Amalgam Elements Penetration into Dental Matrix Using Laser Induced Breakdown Spectroscopy. *J Lasers Med Sci* 2015;6(2):67-73

***Corresponding Author:** Maryam Bahreini, PhD; Laser and Plasma Research Institute, Shahid Beheshti University, G. C., Evin, Tehran, 1983963113, Iran. Tel: +98-2129904018; Fax: +98-2122431775; E-mail: M_Bahreini@sbu.ac.ir

Introduction

Nowadays laser applications in medicine have attracted much more attention and one of these techniques is laser-induced breakdown spectroscopy (LIBS). LIBS is a kind of atomic emission spectroscopic technique which is used for both quantitative and qualitative elemental analysis of any form of the samples.

LIBS techniques proposes plenty of advantages in comparison with other methods for analysis of different biological samples including very tiny amount of sample

(about pico gram) is needed for analysis; the detection limits of this technique are in the limit of few tens of part per million (ppm); This technique can be used to analyze any form of material including solid, liquid and gaseous, and requires a slightly or no preparation of sample^{1,2}; LIBS analysis can be performed in situ or remote as an in vitro or in vivo analytic technique. Other methods including inductively coupled plasma mass spectrometry (ICP-MS)³, atomic absorption spectrophotometry (AAS)⁴, neutron activation analysis (NAA)⁵, x-ray fluorescence (XRF)⁶ and proton particle-induced x-ray emission⁷.

These benefits made it appropriate for the analysis of plenty of biological tissues⁸⁻¹¹ such as bacteria¹², hairs¹³, nails¹⁴⁻¹⁸, bones¹⁹. Samek et al. offered the elemental analysis of tooth samples using LIBS technique for the first time²⁰⁻²². Other groups also reported such application of LIBS in analyzing teeth samples^{23,24}.

In this paper, laser induced breakdown spectroscopy is applied for qualitative analysis of healthy and carious teeth and also amalgam (teeth filling) materials. We propose laser induced breakdown spectroscopy as a quick, real-time and in-situ technique for investigating the proceeding of laser ablation in dentistry including micro-holes drilling and plaque removal. Elemental analysis of healthy and carious teeth and also amalgam materials is done and the penetration of some amalgam elements into dental matrix is investigated. The purpose of this study is to show the capability of LIBS in accurate recognition of healthy and carious teeth within the process of drilling for future clinical applications.

Experimental setup

The experimental setup used for teeth analysis experiments by laser induced breakdown spectroscopy is shown in Figure 1. Neodymium-Doped Yttrium Aluminum Garnet (Nd:YAG) laser pulses with 1064 nm wavelength, 6 ns temporal widths, 2 Hz repetition rate and 90 mJ energy are applied to produce plasma on teeth sample surfaces. The laser pulse is focused on teeth sample by a lens with focal length of 3.5 cm. The samples are located on a XYZ stage and are shifted in a plane perpendicular to the incident laser pulse. So, every laser pulse strikes to the new sample surface. After hitting the focused laser pulse to the sample surface, a hot plasma creates which emits light. The plasma radiation

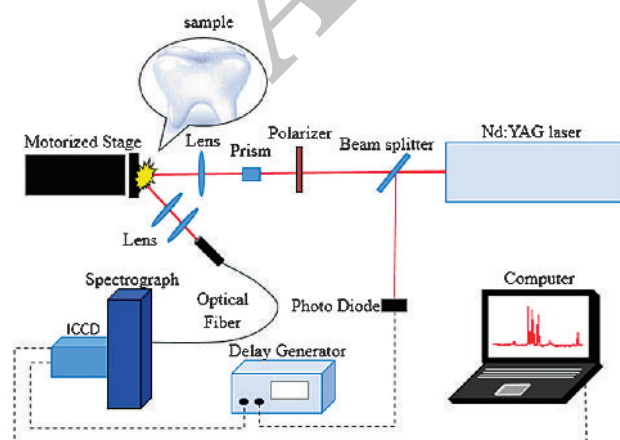


Figure 1. Experimental Setup.

is accumulated by an optical fiber and is sent to the spectrograph. For time resolved detection, an intensified charge-coupled device (ICCD) camera is attached to the spectrograph. A section of laser beam is directed to a photodiode using a beam splitter and then a signal is directed to the delay generator. The optimum delay time of 1 μ s and gate delay width of 20 μ s are selected for the experiments. Therefore, ICCD is triggered using delay generator 1 μ s after the initiation of plasma and every spectrum recorded in 20 μ s.

Sample collection and preparation

The tooth sample is a kind of hard and calcified tissue. Hydroxyapatite is the main matrix material of all calcified tissue. Hydroxyapatite is a crystalline calcium phosphate and its chemical formula is $\text{Ca}_{10}(\text{PO}_4)_6(\text{OH})_2$ ²⁵, but they exhibit some distinct differences. Two different parts of tooth are enamel and dentin (Figure 2). The hardest part of body, enamel, consists of 95% mineral, 4% water and 1% organic material²⁶. The elementary mineral component of enamel is hydroxyapatite. Dentin is the material which is located between enamel and the chamber of pulp. It consists of 70% hydroxyapatite, 10% water and 20% organic material²⁷. So we expect that we will see the intense lines of calcium and phosphorus in the enamel and dentin spectrum, because they are the major element of the basic structure of the hydroxyapatite matrix. Pictures

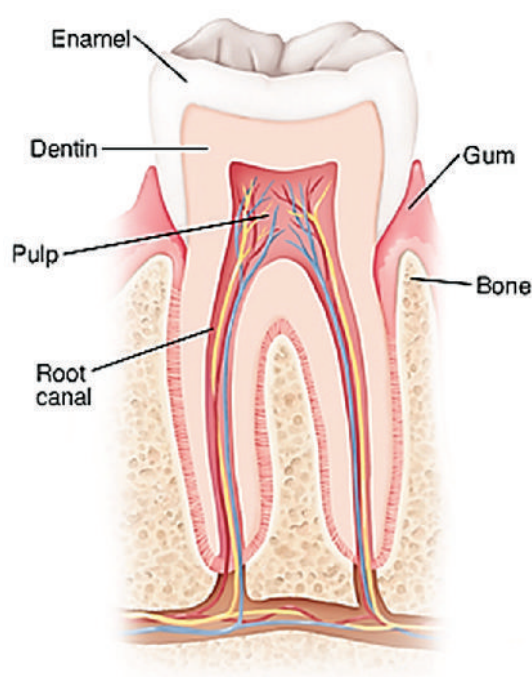


Figure 2. The picture of different sections of a tooth.

of healthy, carious and amalgam filled teeth are shown in Figure 3.

Tooth samples are randomly chosen from elicited permanent tooth of patients of dental school of Shahid Beheshti University in the city of Tehran. No identification was made between the donor and the samples. For bacteria elimination, tooth samples are placed in the solution of %5 sodium hypochlorite for approximately five minutes. Then, for dryness prevention, all samples were placed in distilled water. Before experiments, the samples were dried in the room temperature. After all, they were placed in the experimental setup for LIBS measurements.

Result and discussion

In Figure 4, the tooth after LIBS experiments is shown. As it can be seen, laser pulses ablate very small area of tooth sample and it shows the advantage of this method for dental applications.

A. Elemental analysis of healthy teeth

The LIBS spectrum of healthy enamel is demonstrated in Figure 5. The spectrum is the average of three spectrum

obtained from different points of healthy tissue of teeth. Emission lines are determined by NIST databases. The investigation of teeth spectrum shows that Ca and P are dominant elements and also small quantities of Mg, Na, K, Sr, C, H, Zn, and O can be observed. As it is expected, dominant ionic and atomic emitted lines of Ca and P are identifiers of hydroxyapatite structure of the teeth matrix²⁵.

B. Elemental analysis of carious teeth

The LIBS spectrum of a carious part of tooth is shown in Figure 6. The observed ionic and atomic emission lines of a healthy part of the tooth are also seen in the carious part. However, there are little differences between their intensities.

C. Elemental analysis of amalgam materials

Amalgam is a material which is used to fill the teeth. The LIBS spectrum of filled teeth with amalgam materials is shown in Figure 7. The main amalgam elements including Hg, Ag, Cu and Sn²⁸, emerged in teeth LIBS spectrum.



Figure 3. Pictures of a) healthy, b) carious and c) amalgam filled teeth.

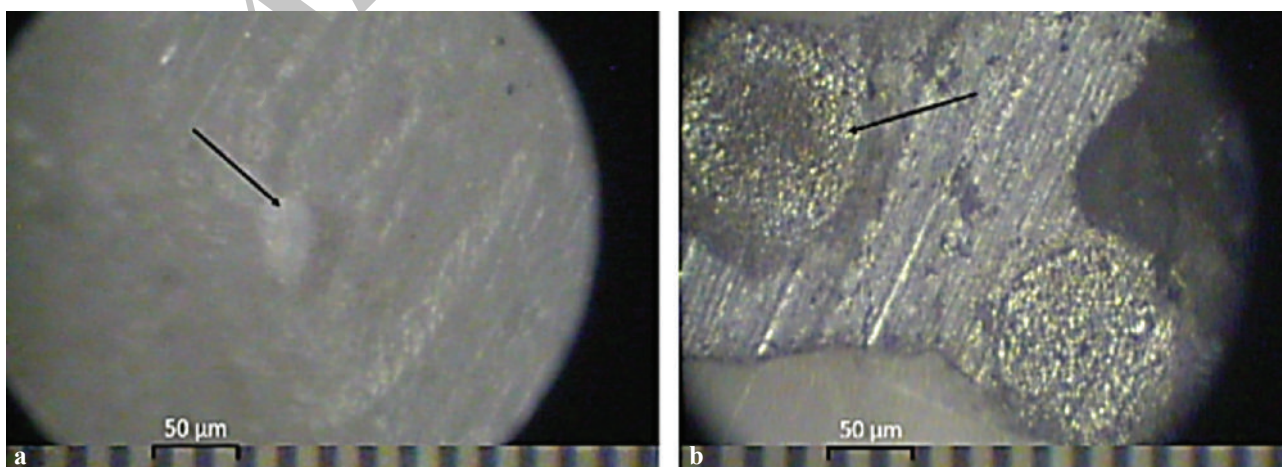


Figure 4. Microscopic image indicating ablation locations in teeth after LIBS experiments: a) healthy b) amalgam filled tissue.

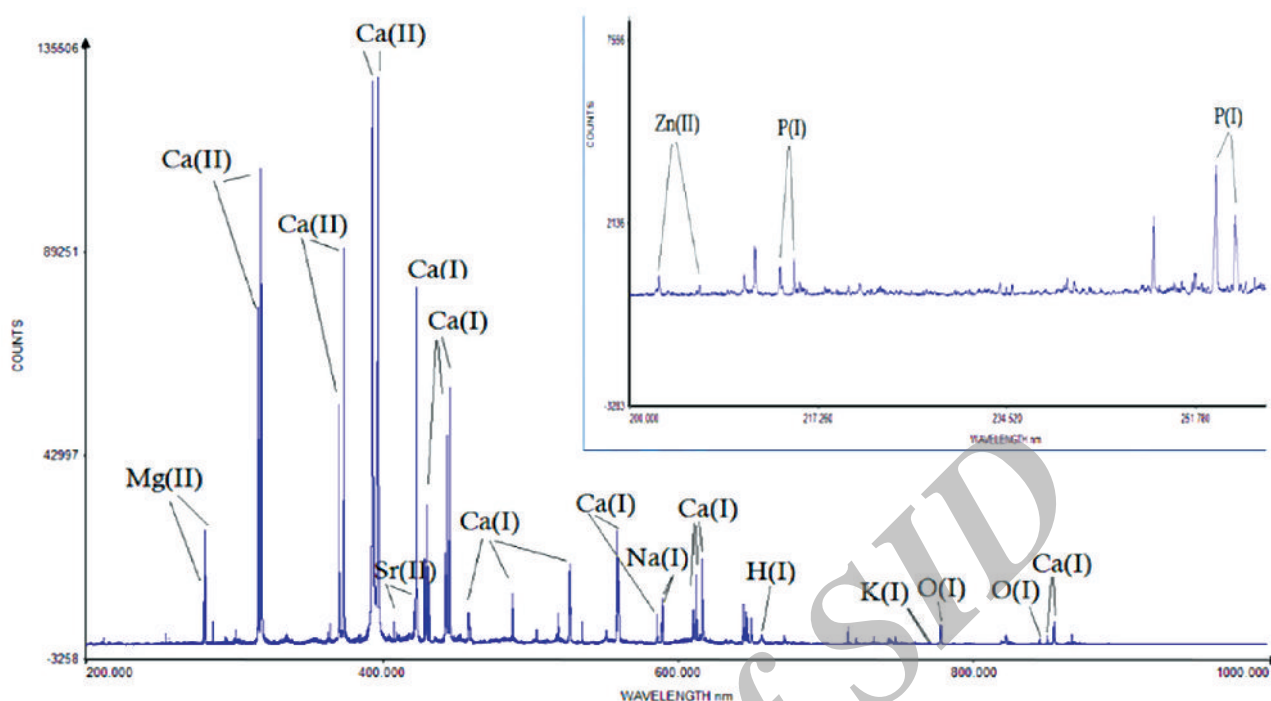


Figure 5. LIBS spectrum of healthy part of tooth.

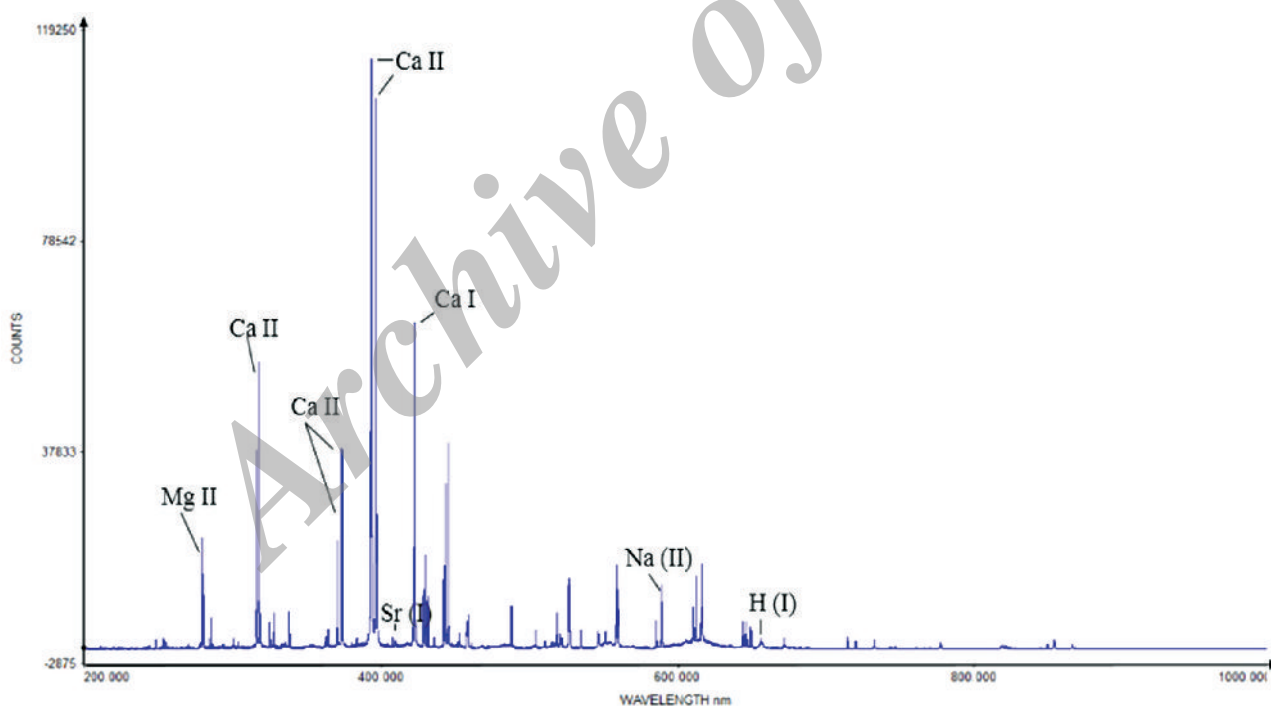


Figure 6. LIBS spectrum of carious part of tooth.

D. Penetration of amalgam elements into dental matrix

As it is mentioned, the main amalgam elements are Hg, Ag, Cu and Sn. Accumulation of some of these elements, for example Hg, has toxic effects in human tissue²⁹. As

the LIBS method can analyze the samples spatially, we used it in order to investigate the penetration of amalgam elements into dental matrix. To do this, we cut the tooth in a cross-sectional way. By investigating the resulted spectrum from different points of this cross section, it can be seen that amalgam elements have remarkable

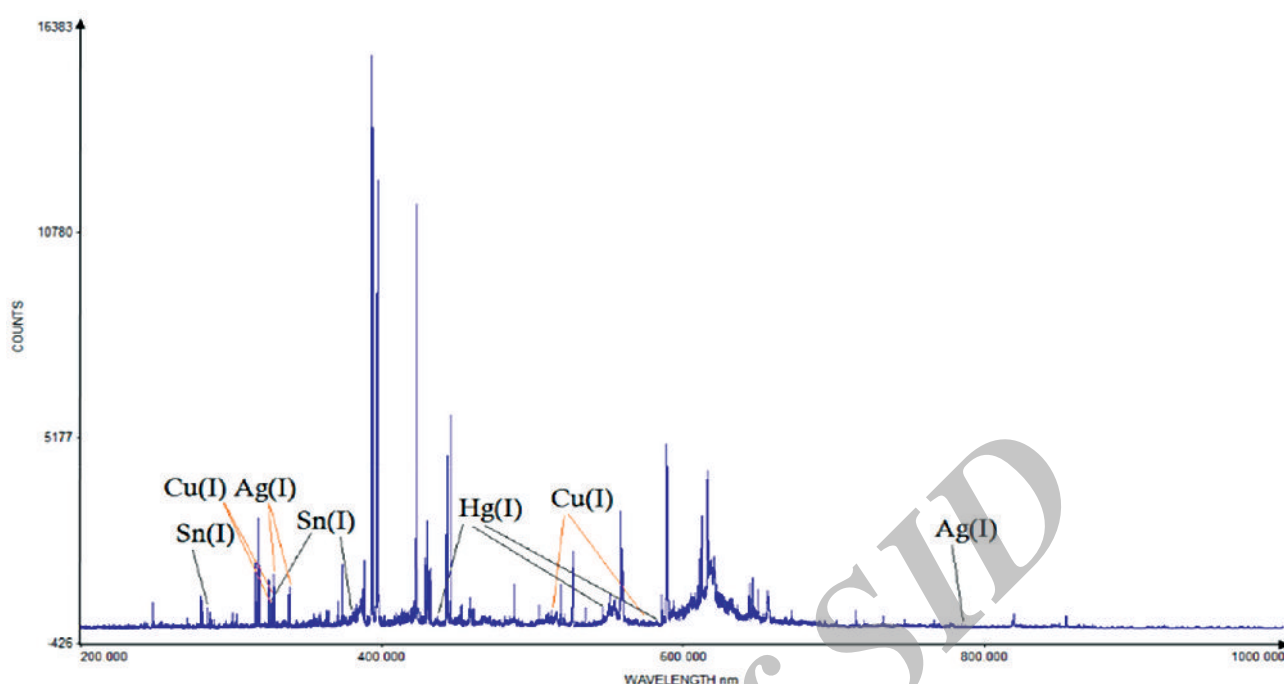


Figure 7. LIBS spectrum of amalgam filled tooth.

penetration in other part of tooth matrix. By going away from filled center, the penetration of amalgam elements is reduced. The same results have been achieved when investigating one point of tooth by moving from surface to inside. As it is shown in Figure 8, the more laser pulse went into the tooth, the more reduced the existence of amalgam elements.

Conclusion

Laser induced breakdown spectroscopy (LIBS) technique is performed for qualitative analysis of healthy and carious parts of the teeth to investigate the possible utilization during the teeth treatment of micro-holes drilling and plaque removal. We propose laser induced breakdown spectroscopy as an in situ, quick and easy

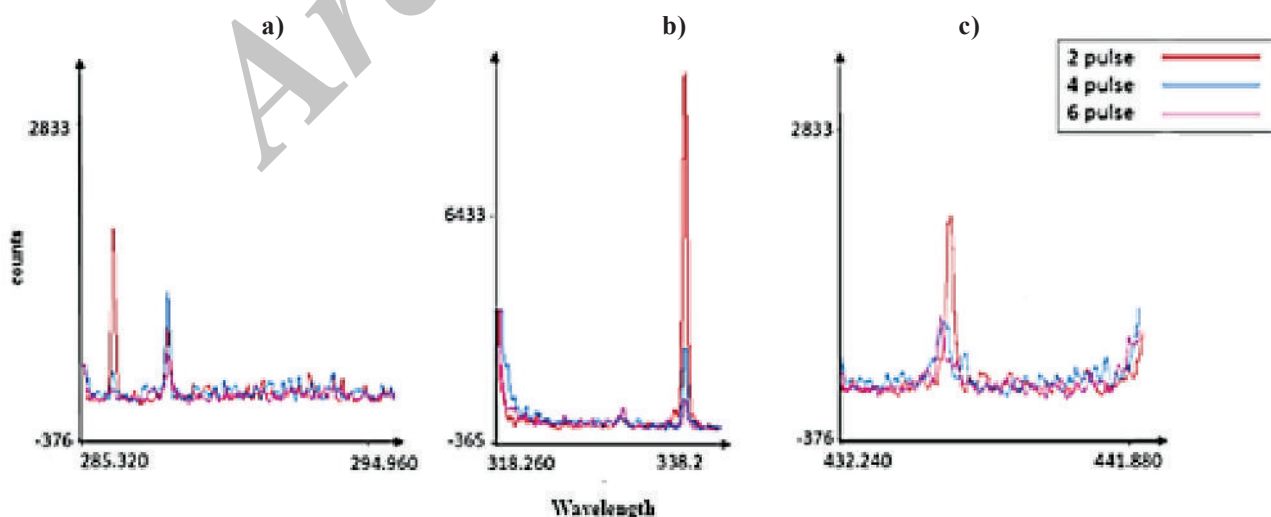


Figure 8. Different regions of LIBS spectra of one point of teeth obtained by moving from surface to inside were related to these elements: a) Sn I (283.9), b) Ag I (338.2) and c) Hg I (435.8).

technique for drilling process monitoring. The results of elemental analysis show the presence of some trace elements in teeth including P, Ca, Mg, Zn, K, Sr, C, Na, H, O. Elemental analysis of teeth filling material including Hg, Ag, Cu and Sn and the possibility of their penetration into the healthy tissue of tooth matrix is also studied. This study addresses the ability of LIBS in elemental analysis of teeth and its possibility in clinical utilization in valuable discrimination of healthy and carious teeth within the process of drilling and preventing from omitting some parts of carious tissue.

Acknowledgement

The authors would like to thank every person in Dental School of Shahid Beheshti University of Medical Sciences for their friendly support in tooth samples collection.

References

1. Cremers DA, Radziemski LJ. Handbook of Breakdown Spectroscopy, 1th ed. Chichester, Wiley. 2006. pp 1-5.
2. Singh JP, Thakur SN. Laser induced breakdown spectroscopy, 1th ed. New York, Elsevier. 2007. pp 313-314.
3. Goullé JP, Saussereau E, Mahieu L, Bouige D, Groenwout S, Guerbet M, et al. Application of inductively coupled plasma mass spectrometry multielement analysis in fingernail and toenail as a biomarker of metal exposure. *J Anal Toxicol*. 2009; 33(2): 92-8.
4. Ohgita S, Fujita T, Fujii Y, Hayashi C, Nishio H. Nail calcium and magnesium content in relation to age and bone mineral density. *J Bone Miner Metab*. 2005; 23(4): 318-22.
5. Fell GS, Smith H, Howie RA. Neutron activation analysis for copper in biological material applied to Wilson's disease. *J Clin Pathol*. 1968; 21(1):8-11.
6. Baranowska L, Barchański L, Bąk M, Smolec B, Mzyk Z. X-Ray Fluorescence Spectrometry in Multielemental Analysis of Hair and Teeth. *J Environ Stud*. 2004; 13(6): 639-46.
7. Biswas SK, Abdullah M, Akhter S, Tarafdar SA, Khaliqzaman M, Khan AH. Trace elements in human fingernails: Measurement by proton-induced X-ray emission. *J Radioanal Nucl Chem*. 1983; 1: 111-24.
8. Rehse SJ, Salimnia H, Miziolek AW. Laser-induced breakdown spectroscopy (LIBS): an overview of recent progress and future potential for biomedical applications. *J Med Eng Technol*. 2012; 36(2): 77-89.
9. Singh VK, Rai A. Prospects for laser-induced breakdown spectroscopy for biomedical applications: a review. *Lasers Med Sci*. 2011; 26(5): 673-87.
10. Assion A, Wollenhaupt M, Haag L, Mayorov F, Sarpe-Tudoran C, Winter M, et al. Femtosecond laser-induced-breakdown spectrometry for Ca 2+ analysis of biological samples with high spatial resolution. *Appl Phys B Lasers Opt*. 2003; 77(4): 391-7.
11. Abdel-Salam ZA, Nanjing Z, Anglos D, Harith MA. Effect of experimental conditions on surface hardness measurements of calcified tissues via LIBS. *Appl Phys B*. 2008; 94(1) 141-7.
12. Baudelet M, Yu J, Bossu M, Jovelet J, Wolf JP, Amodeo Y, et al. Discrimination of microbiological samples using femtosecond laser-induced breakdown spectroscopy. *Appl Phys Lett*. 2006; 89(16): 163903.
13. Corsi M, Cristoforetti G, Hidalgo M, Legnaioli S, Palleschi V, Salvetti A, et al. Application of laser-induced breakdown spectroscopy technique to hair tissue mineral analysis. *Appl Opt*. 2003. 42(30): 6133-7.
14. Hosseinimakarem Z, Tavassoli SH. Analysis of human nails by laser-induced breakdown spectroscopy. *J Biomed Opt*. 2011; 16(5): 057002.
15. Shadman S, Bahreini M, Tavassoli SH. Comparison between elemental composition of human fingernails of healthy and opium-addicted subjects by laser-induced breakdown spectroscopy. *Appl. Opt*. 2012; 51(12): 2004-11.
16. Bahreini M, Hosseinimakarem Z, Hassan Tavassoli S. A study of association between fingernail elements and osteoporosis by laser-induced breakdown spectroscopy. *J Appl Phys*. 2012; 112(5): 054701.
17. Bahreini M, Tavassoli SH. Possibility of Thyroidism Diagnosis by Laser Induced Breakdown Spectroscopy of Human Fingernail. 2012; 3(3): 127-31.
18. Bahreini M, Ashrafxhani B, Tavassoli SH. Elemental analysis of fingernail of alcoholic and doping subjects by laser-induced breakdown spectroscopy. *Appl Phys B*. 2013; 114(3): 439-47.
19. Kasem MA, Russo RE, Harith MA. Influence of biological degradation and environmental effects on the interpretation of archeological bone samples with laser-induced breakdown spectroscopy. *J Anal At Spectrom*. 2011; 26(9): 1733.
20. Samek O, Beddows DCS, Telle HH, Morris GW, Liska M, Kaiser J. Quantitative analysis of trace metal accumulation in teeth using laser-induced breakdown spectroscopy. 1999; 69(1): 179-82.
21. Samek O, Liska M, Kaiser J, Beddows DCS, Telle HH, Kulkhlevsky SV. Clinical application of laser-induced breakdown spectroscopy to the analysis of teeth and dental materials. *J Clin Laser Med Surg*. 2000; 18(6): 281-9.
22. Samek O, Beddows DCS, Telle HH, Kaiser J, Liska M, Cáceres JO, et al. Quantitative laser-induced breakdown spectroscopy analysis of calcified tissue samples. 2001; 56(6): 865-75.
23. Thareja RK, Sharma AK, Shukla S. Spectroscopic investigations of carious tooth decay. *Med Eng Phys*. 2008; 30(9): 1143-8.
24. Singh VK, Rai AK. Potential of laser-induced breakdown spectroscopy for the rapid identification of carious teeth. *Lasers Med Sci*. 2011; 26(3): 307-15.
25. Hutt L, Zealand N. Spherical indentation of tooth enamel. *J Mater Sci*. 1981; 16: 2551-6.

26. Nancy A. Ten Cate's Oral Histology, 8th ed. Elsevier. 2013. p12-63.
27. Nanci, Ten Cate's Oral Histology, 8th ed. Elsevier. 2013. p 163.
28. Jack L. Ferracane MS PhD FADM, Materials in Dentistry: Principles and Applications, 2th ed. Lippincott Williams & Wilkins. 2001.pp 119-127.
29. Samek O, Lika M, Kaiser J, Krzyánek V, Beddows DCS, Belenkevitch A, et al. Laser ablation for mineral analysis in the human body: integration of LIFS with LIBS. Proc. SPIE 3570, Biomedical Sensors, Fibers, and Optical Delivery Systems, 263-71 (January 15, 1999); doi:10.1117/12.336941.

Archive of SID